

FIG. 1

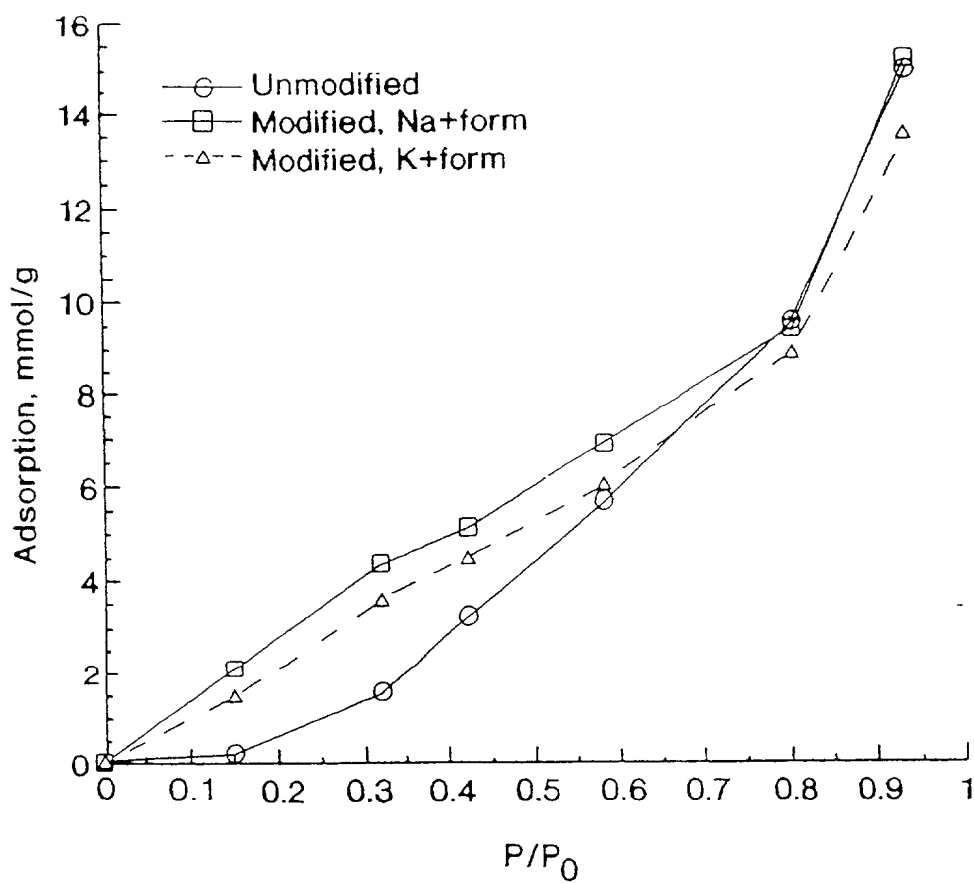


FIG. 2

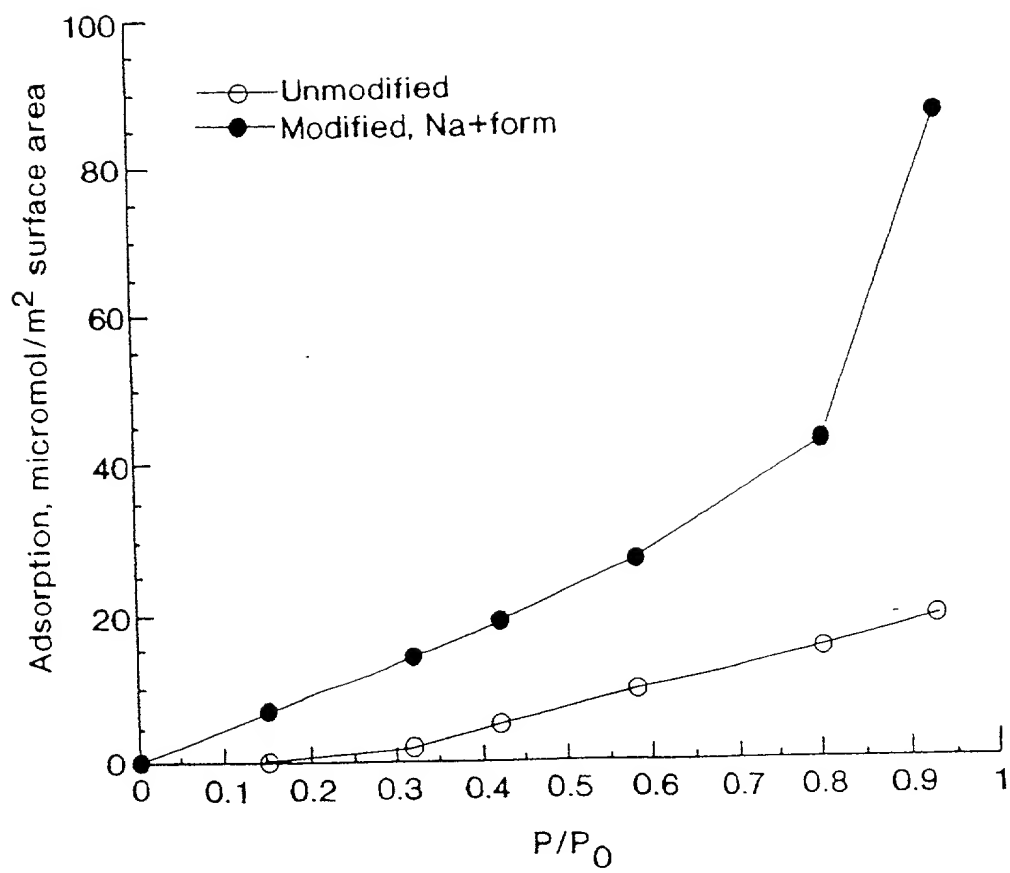


FIG. 3

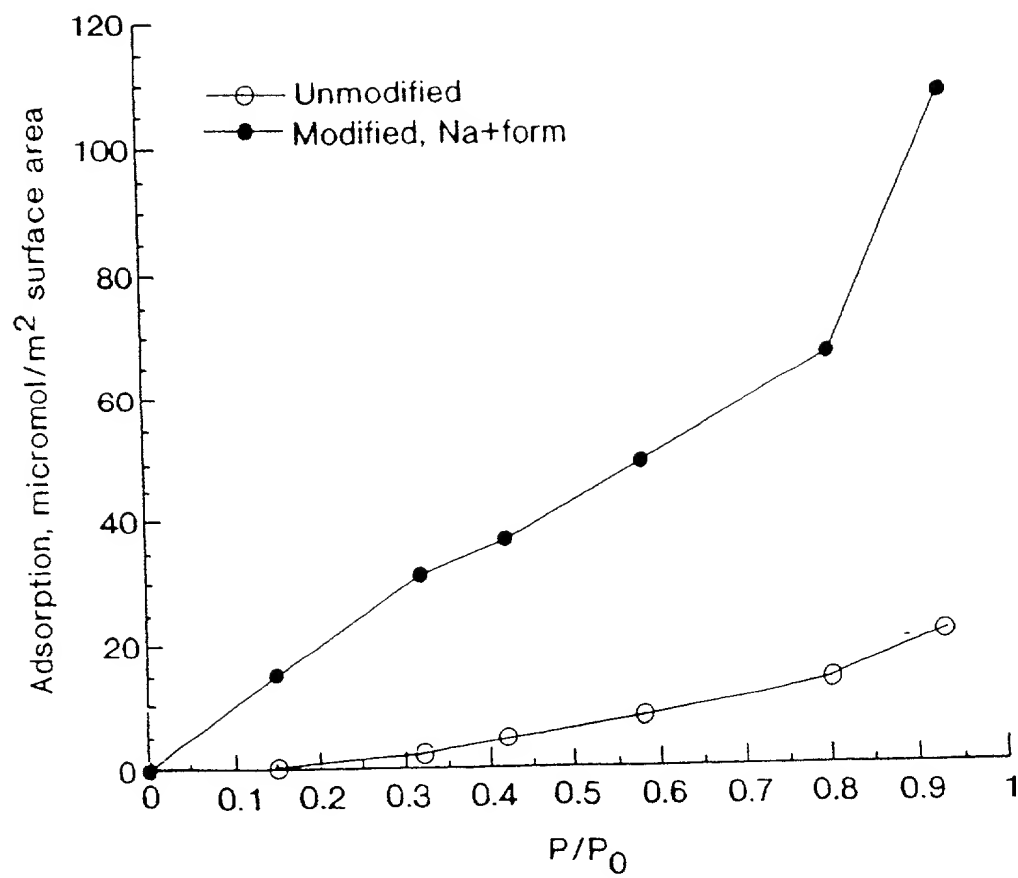


FIG. 4

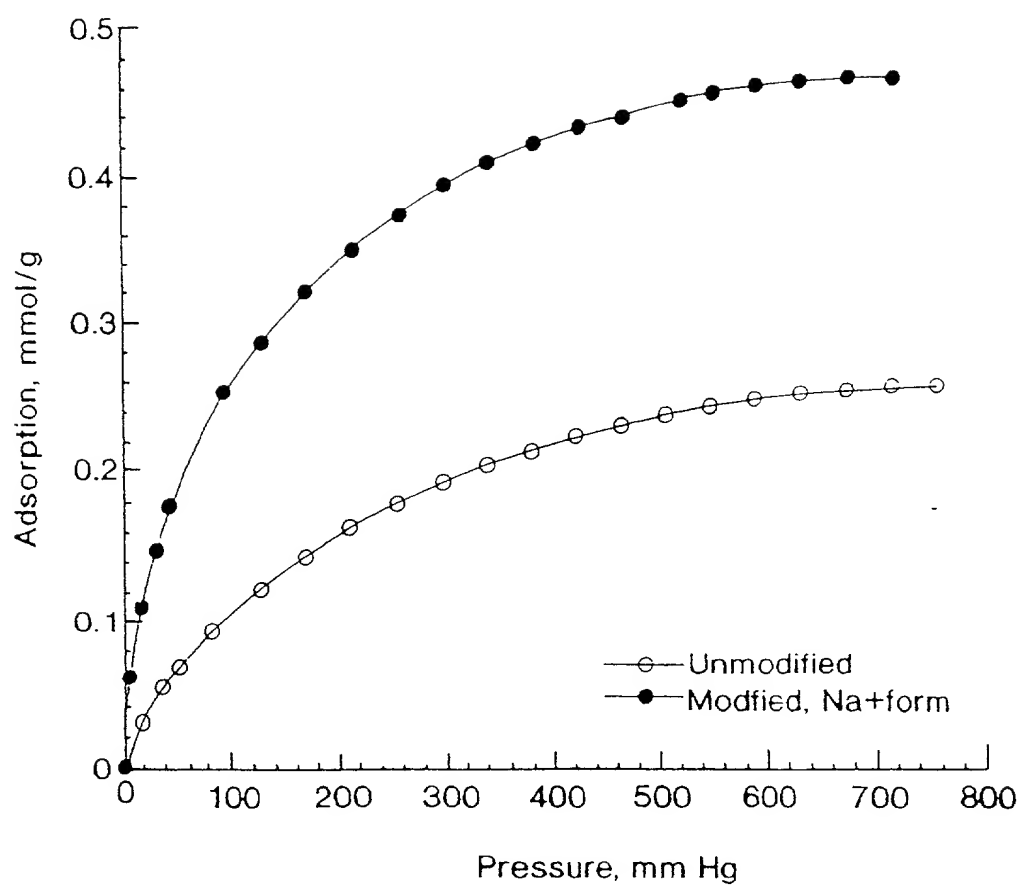


FIG. 5


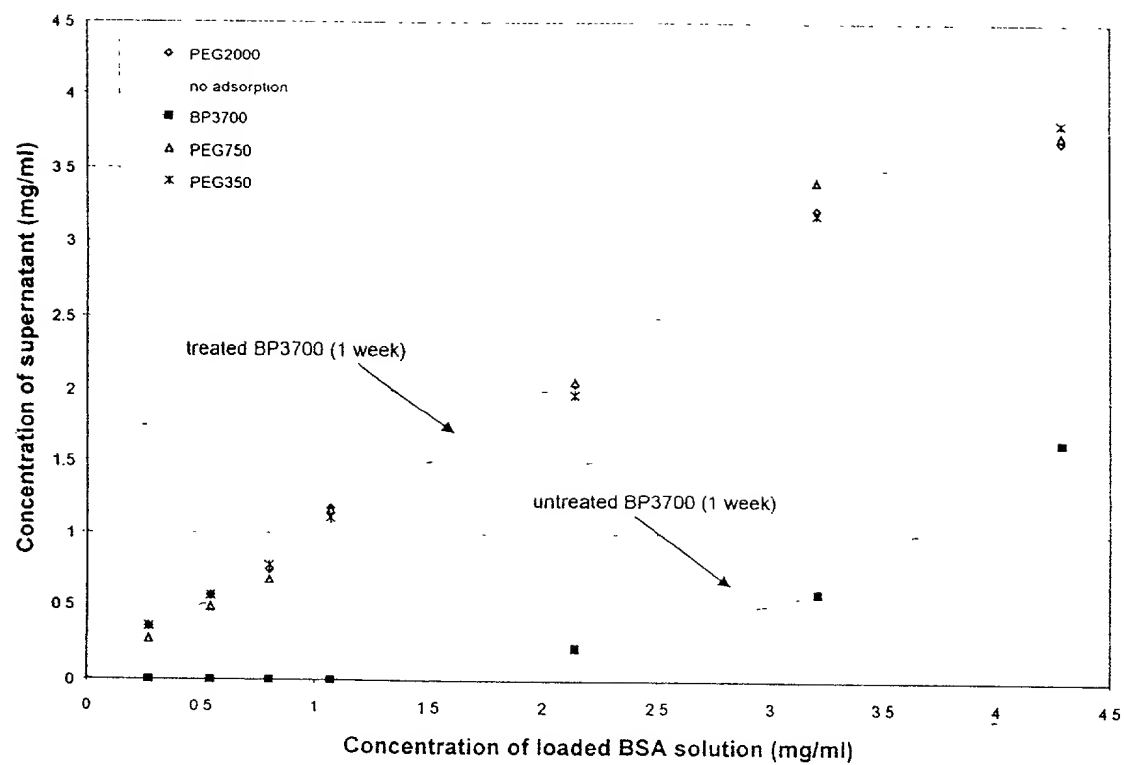


FIG. 6

Separation of Barbiturates

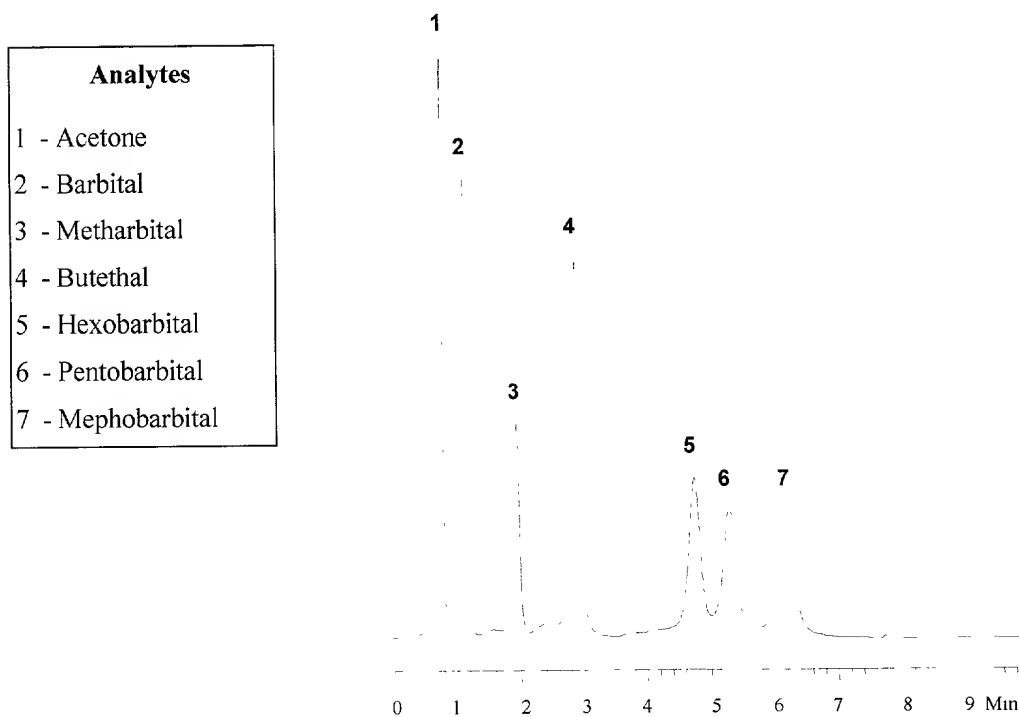

LC Conditions

Column: 50 x 4.6 mm

Mobile Phase: 20/80 A/B

A: ACN

B: 20 mM Ammonium phosphate, pH 7.0

Flow rate: 1.0 mL/min.

Temperature: 30 °C

Injection volume: 5 µL

Detection: 254 nm

Figure 7. Separation of barbiturates using a 50x4.6 mm HPLC column packed with SP-2.

Figure 7

Separation of PTH-Amino Acids

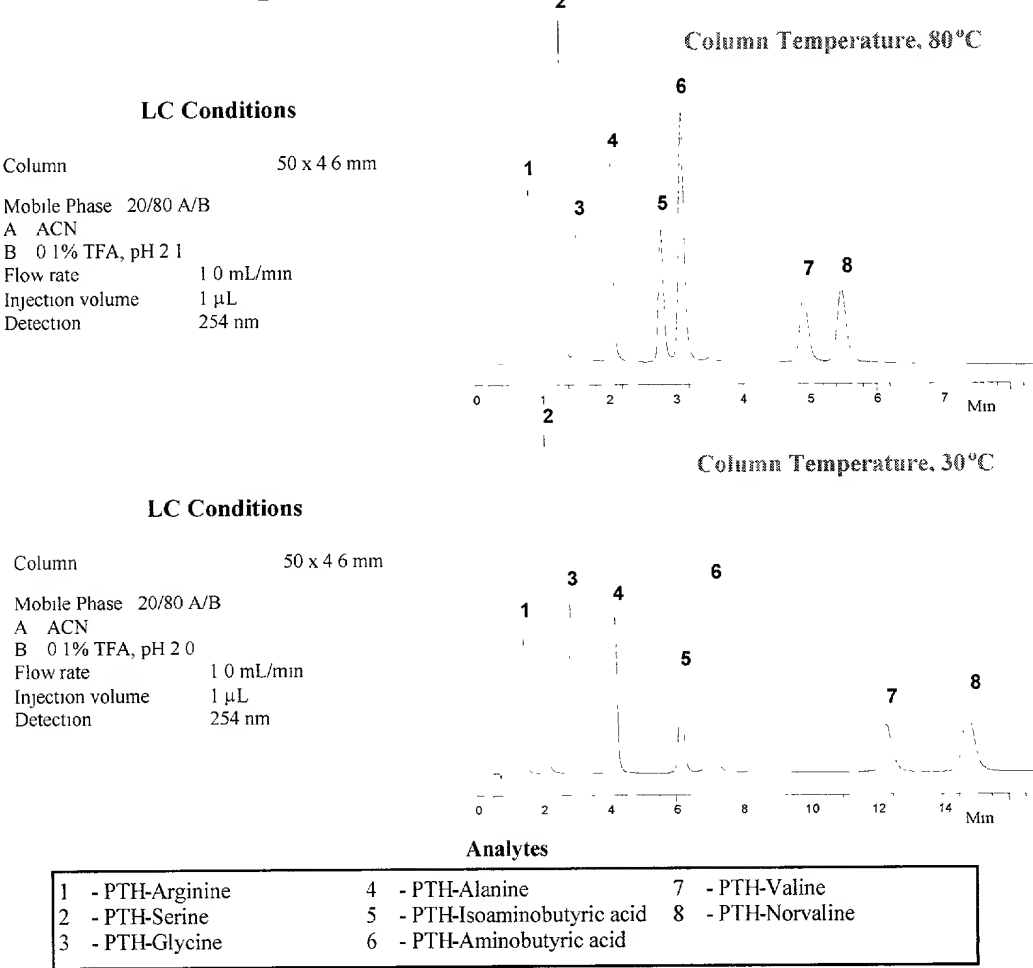


Figure 8. Separation of PTH Aminoacids using a 50x4.6 mm HPLC column packed with SP-2.

Figure 8

Separation of NSAID's

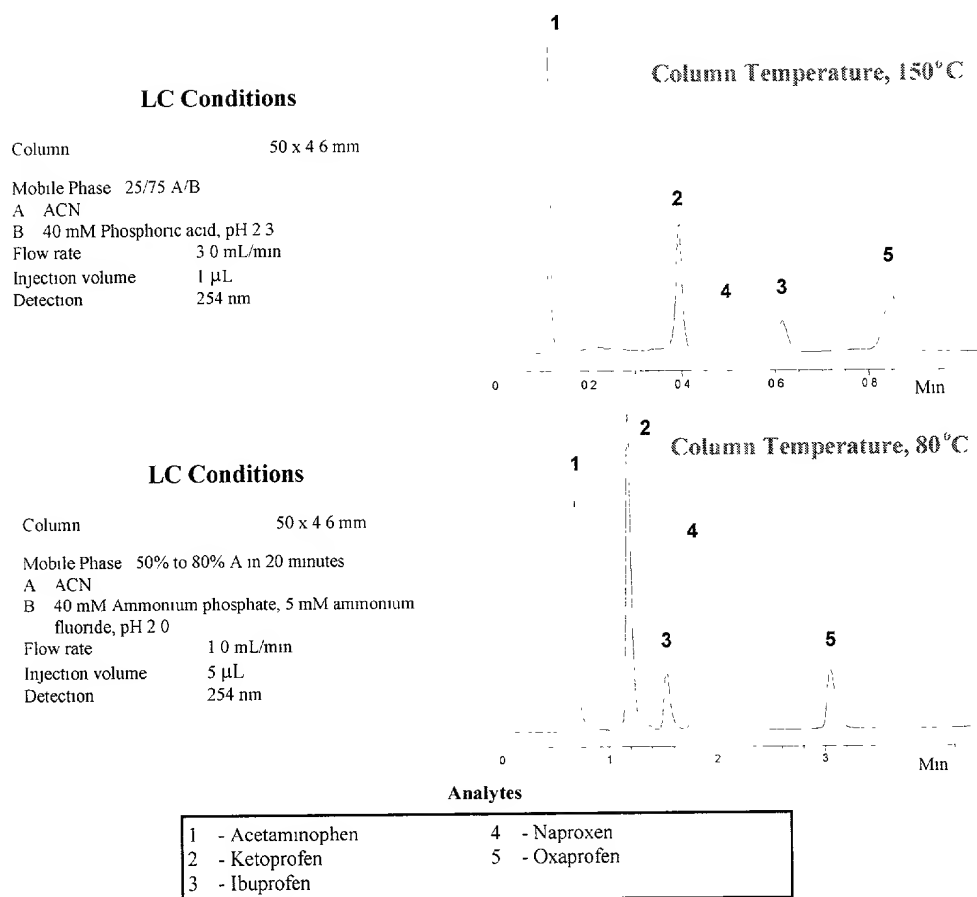


Figure 9. Separation of non steroidal anti-inflammatory drugs using a 50x4.6 mm HPLC column packed with SP-2.

Figure 9

Separation of Ethylbenzene and p-Xylene

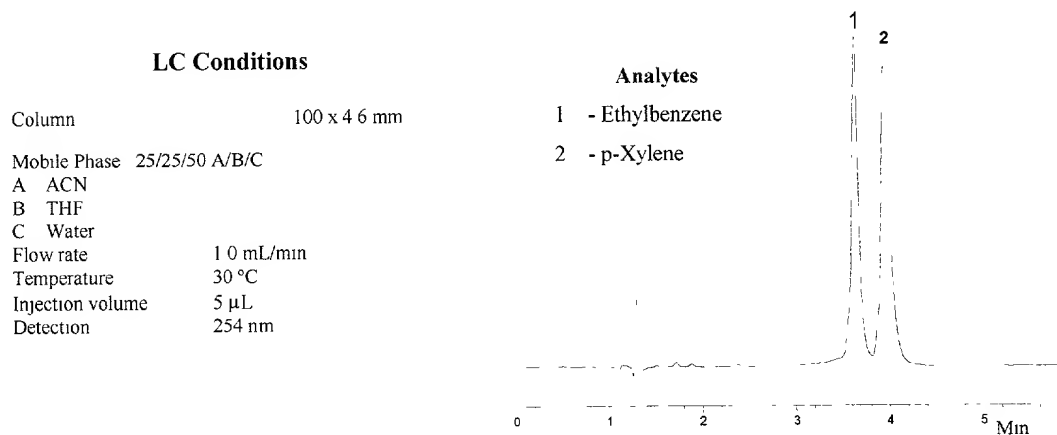


Figure 10. Separation of p-xylene and ethylbenzene using a 100x4.6 mm HPLC column packed with SP-2.

Figure 10

Separation of Beta-Blockers

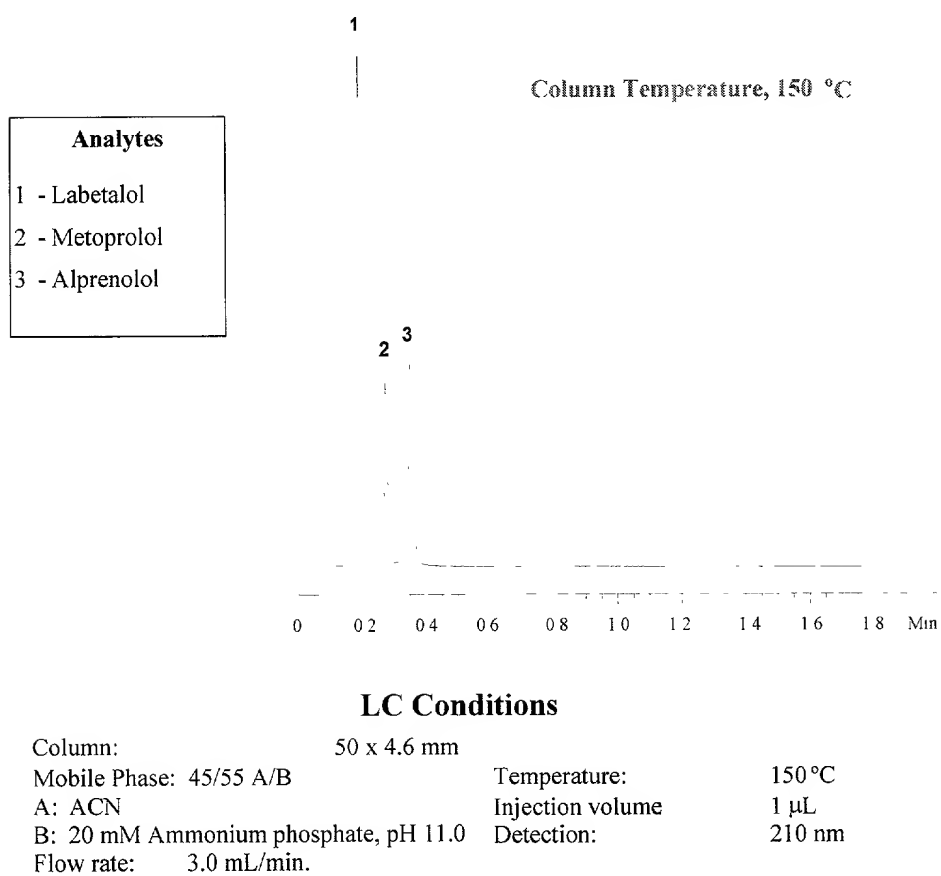


Figure 11. Separation of beta-blockers using a 50 x 4.6 mm HPLC column packed with SP-2.

Figure 11